

**IMPORTANT: Please read carefully and keep this information for future use.**

**This Package Insert and Fitting Guide is intended for the Eye Care Professional, but should be made available to patients upon request.**

**The Eye Care Professional should provide the patient with the appropriate instructions that pertain to the patient's prescribed lenses. Copies are available for download at [www.acuvue.com](http://www.acuvue.com).**

# ACUVUE®

## OASYS

BRAND CONTACT LENSES

**ACUVUE OASYS® Brand Contact Lenses**

**ACUVUE OASYS® Brand Contact Lenses for ASTIGMATISM**

**ACUVUE OASYS® Brand Contact Lenses for PRESBYOPIA**













**senofilcon A Soft (hydrophilic) Contact Lenses  
Visibility Tinted with UV Blocker  
for Daily and Extended Wear**



CAUTION: U.S. Federal law restricts this device to sale by or on the order of a licensed practitioner.

# SYMBOLS KEY

The following symbols may appear on the label or carton:

SYMBOL	DEFINITION
	Consult Instructions for Use
	Manufactured by or in
	Date of Manufacture
	Use By Date (expiration date)
	Batch Code
	Sterile Using Steam or Dry Heat
<b>DIA</b>	Diameter
<b>BC</b>	Base Curve
<b>D</b>	Diopter (lens power)
<b>CYL</b>	Cylinder
<b>AXIS</b>	Axis
<b>MAX ADD</b>	Near ADD
<b>LOW</b>	“Low” Near ADD
<b>MID</b>	“Medium” Near ADD
<b>HGH</b>	“High” Near ADD
	Quality System Certification Symbol
	UV-Blocking
	Fee Paid for Waste Management
	CAUTION: U.S. Federal law restricts this device to sale by or on the order of a licensed practitioner
	Lens Orientation Correct
	Lens Orientation Incorrect (Lens Inside Out)

# DESCRIPTION

The ACUVUE OASYS® Brand Contact Lenses, the ACUVUE OASYS® Brand Contact Lenses for ASTIGMATISM, and the ACUVUE OASYS® Brand Contact Lenses for PRESBYOPIA are soft (hydrophilic) contact lenses available as spherical, toric, or multifocal lenses and include HYDRACLEAR® PLUS Technology. The lenses are made of a silicone hydrogel material containing an internal wetting agent with visibility tinted UV absorbing monomer.

These lenses are tinted blue using Reactive Blue Dye #4 to make the lenses more visible for handling. A benzotriazole UV absorbing monomer is used to block UV radiation.

The transmittance characteristics are less than 1% in the UVB range of 280 nm to 315 nm and less than 10% in the UVA range of 316 nm to 380 nm for the entire power range.

## Lens Properties:

- Specific Gravity (calculated): 0.98 – 1.12
- Refractive Index: 1.42
- Light Transmittance: 85% minimum
- Surface Character: Hydrophilic
- Water Content: 38%
- Oxygen Permeability:

### VALUE

$103 \times 10^{-11}$  (cm<sup>2</sup>/sec)  
(ml O<sub>2</sub>/ml x mm Hg) @ 35°C

$122 \times 10^{-11}$  (cm<sup>2</sup>/sec)  
(ml O<sub>2</sub>/ml x mm Hg) @ 35°C

### METHOD

Fatt (boundary corrected, edge corrected)

Fatt (boundary corrected, non-edge corrected)

## Lens Parameters:

- Diameter Range: 12.0 mm to 15.0 mm
- Center Thickness: varies with power
- Base Curve Range: 7.85 mm to 10.00 mm
- Spherical Power Range: Daily Wear: -20.00D to +20.00D  
Extended Wear: -20.00D to +14.00D
- Multifocal ADD Power Range: +0.25D to +4.00D
- Cylinder Power Range: -0.25D to -10.00D
- Axis Range: 2.5° to 180°

# AVAILABLE LENS PARAMETERS

The ACUVUE OASYS® Brand Contact Lenses are hemispherical shells of the following dimensions:

<b>Diameter:</b>	14.0 mm
<b>Center Thickness:</b>	Minus Lens - varies with power (e.g. -4.00D: 0.070 mm) Plus Lens - varies with power (e.g. +4.00D: 0.168 mm)
<b>Base Curve:</b>	8.4 mm, 8.8 mm
<b>Powers:</b>	-0.50D to -6.00D (in 0.25D increments) -6.50D to -12.00D (in 0.50D increments) +0.50D to +6.00D (in 0.25D increments) +6.50D to +8.00D (in 0.50D increments)

The ACUVUE OASYS® Brand Contact Lenses for ASTIGMATISM are hemitoric shells of the following dimensions:


<b>Diameter:</b>	14.5 mm
<b>Center Thickness:</b>	Minus Lens - varies with power (e.g. -4.00D: 0.080 mm) Plus Lens - varies with power (e.g. +4.00D: 0.172 mm)
<b>Base Curve:</b>	8.6 mm
<b>Powers:</b>	plano to -6.00D (in 0.25D increments) -6.50D to -9.00D (in 0.50D increments) +0.25D to +6.00D (in 0.25D increments)  Cylinder: -0.75D, -1.25D, -1.75D, -2.25D, -2.75D  Axis: 10° to 180° (in 10° increments)

The ACUVUE OASYS® Brand Contact Lenses for PRESBYOPIA are hemispherical shells of the following dimensions:

<b>Diameter:</b>	14.3 mm
<b>Center Thickness:</b>	Minus Lens - varies with power (e.g. -4.00D: 0.070 mm) Plus Lens - varies with power (e.g. +4.00D: 0.168 mm)
<b>Base Curve:</b>	8.4 mm
<b>Powers:</b>	-9.00D to +6.00D (in 0.25D increments)
<b>ADD Powers:</b>	+1.25 (LOW), +1.75 (MID), +2.50 (HGH)

# TRANSMITTANCE CURVE

ACUVUE OASYS® Brand Contact Lenses vs. 24 yr. old human cornea vs. 25 yr. old human crystalline lens

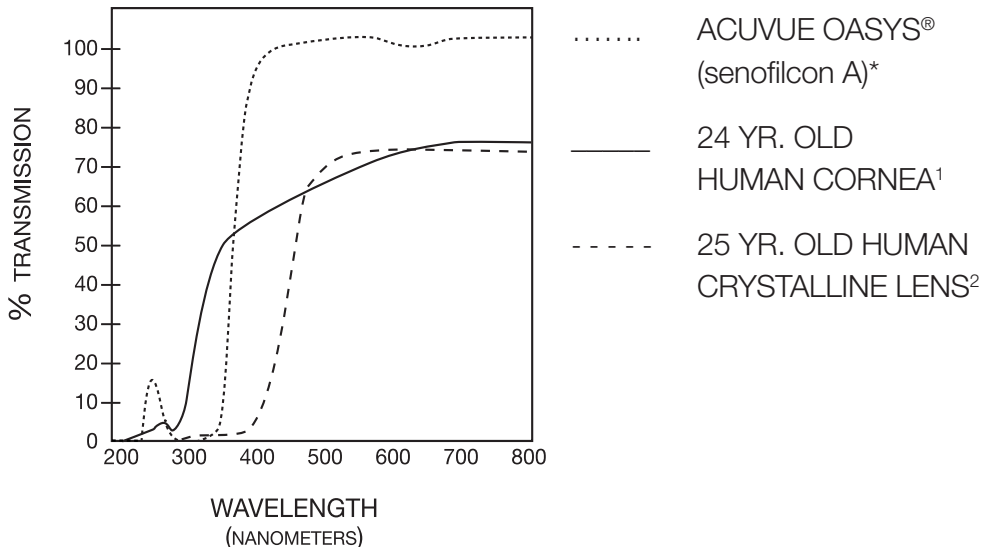

\*The data was obtained from measurements taken through the central 3-5 mm portion for the thinnest marketed lens (-1.00D lens, 0.070 mm center thickness).

1. Lerman, S., Radiant Energy and the Eye, MacMillan, New York, 1980, p.58, figure 2-21

2. Waxler, M., Hitchins, V.M., Optical Radiation and Visual Health, CRC Press, Boca Raton, Florida, 1986, p.19, figure 5

**WARNING: UV absorbing contact lenses are NOT substitutes for protective UV absorbing eyewear, such as UV absorbing goggles or sunglasses because they do not completely cover the eye and surrounding area. The patient should continue to use UV absorbing eyewear as directed.**

## ACTIONS

In its hydrated state, the contact lens, when placed on the cornea, acts as a refracting medium to focus light rays on the retina. When hydrated and placed on the cornea for therapeutic use, the contact lens acts as a bandage to protect the cornea.

The transmittance characteristics are less than 1% in the UVB range of 280 nm to 315 nm and less than 10% in the UVA range of 316 nm to 380 nm for the entire power range.

**NOTE: Long-term exposure to UV radiation is one of the risk factors associated with cataracts. Exposure is based on a number of factors such as environmental conditions (altitude, geography, cloud cover) and personal factors (extent and nature of outdoor activities). UV-Blocking contact lenses help provide protection against harmful UV radiation.**

**However, clinical studies have not been done to demonstrate that wearing UV-Blocking contact lenses reduces the risk of developing cataracts or other eye disorders. The Eye Care Professional should be consulted for more information.**

## INDICATIONS (USES)

The ACUVUE OASYS® Brand Contact Lens is indicated for the optical correction of refractive ametropia (myopia and hyperopia) in phakic or aphakic persons with non-diseased eyes who have 1.00D or less of astigmatism.

The ACUVUE OASYS® Brand Contact Lens for ASTIGMATISM is indicated for the optical correction of visual acuity in phakic or aphakic persons with non-diseased eyes that are hyperopic or myopic and may have 10.00D or less of astigmatism.

The ACUVUE OASYS® Brand Contact Lens for PRESBYOPIA is indicated for the optical correction of distance and near vision in presbyopic, phakic or aphakic persons with non-diseased eyes who may have 0.75D or less of astigmatism.

These lenses contain a UV Blocker to help protect against transmission of harmful UV radiation to the cornea and into the eye.

Eye Care Professionals may prescribe the lenses either for single-use disposable wear or frequent/planned replacement wear with cleaning, disinfection and scheduled replacement (see "REPLACEMENT SCHEDULE"). When prescribed for frequent/planned replacement wear, the lenses may be cleaned and disinfected using a chemical disinfection system only.

These lenses have been approved for daily and extended wear for up to 6 nights/7 days of continuous wear. It is recommended that the contact lens wearer first be evaluated on a daily wear schedule. If successful, then a gradual introduction of extended wear can be followed as determined by the prescribing Eye Care Professional.

These lenses are also indicated for therapeutic use as a bandage lens for the following acute and chronic ocular conditions:

- For corneal protection in lid and corneal abnormalities such as entropion, trichiasis, tarsal scars, and recurrent corneal erosion. In addition, they are indicated for protection where sutures or ocular structure malformation, degeneration or paralysis may result in the need to protect the cornea from exposure or repeated irritation.
- For corneal pain relief in conditions such as bullous keratopathy, epithelial erosion and abrasion, filamentary keratitis, and post-keratoplasty.
- For use as a barrier during the healing process of epithelial defects such as chronic epithelial defects, corneal ulcer, neurotrophic and neuroparalytic keratitis, and chemical burns.
- For post surgical conditions where bandage lens use is indicated such as post refractive surgery, lamellar grafts, corneal flaps, and additional ocular

surgical conditions.

- For structural stability and protection in piggy back lens fitting where the cornea and associated surfaces are too irregular to allow for corneal rigid gas permeable (RGP) lenses to be fit. In addition, the use of the lens can prevent irritation and abrasions in conditions where there are elevation differences in the host/graph junction or scar tissue.

Lenses prescribed for therapeutic use may be worn for daily or extended wearing periods.

## CONTRAINDICATIONS (REASONS NOT TO USE)

When prescribing contact lens wear for REFRACTIVE AMETROPIA USE, DO NOT USE these lenses when any of the following conditions exist:

- Acute or subacute inflammation or infection of the anterior chamber of the eye
- Any eye disease, injury or abnormality that affects the cornea, conjunctiva or eyelids
- Severe insufficiency of lacrimal secretion (dry eye)
- Corneal hypoesthesia (reduced corneal sensitivity)
- Any systemic disease that may affect the eye or be exaggerated by wearing contact lenses
- Allergic reactions of ocular surfaces or adnexa that may be induced or exaggerated by wearing contact lenses or use of contact lens solutions
- Ocular irritation due to allergic reactions which may be caused by use of contact lens solutions (i.e., cleaning and disinfecting solutions, rewetting drops, etc.) that contain chemicals or preservatives (such as mercury or Thimerosal, etc.) to which some people may develop an allergic response
- Any active corneal infection (bacterial, fungal, protozoal or viral)
- If eyes become red or irritated

For THERAPEUTIC USE, the Eye Care Professional may prescribe these lenses to aid in the healing process of certain ocular conditions, which may include those cited above.

## WARNINGS

**Patients should be advised of the following warnings pertaining to contact lens wear:**

**EYE PROBLEMS, INCLUDING CORNEAL ULCERS, CAN DEVELOP RAPIDLY AND LEAD TO LOSS OF VISION; IF THE PATIENT EXPERIENCES:**

- **Eye Discomfort,**
- **Excessive Tearing,**

- **Vision Changes,**
- **Loss of Vision,**
- **Eye Redness,**
- **Or Other Eye Problems,**

**THE PATIENT SHOULD BE INSTRUCTED TO IMMEDIATELY REMOVE THE LENSES AND PROMPTLY CONTACT THE EYE CARE PROFESSIONAL.**

- When prescribed for daily wear, patients should be instructed not to wear lenses while sleeping. Clinical studies have shown that the risk of serious adverse reactions is increased when lenses are worn overnight, and that the risk of ulcerative keratitis is greater for extended wear contact lens users than for daily wear users.<sup>3</sup>
- Studies have shown that contact lens wearers who are smokers have a higher incidence of adverse reactions than nonsmokers.
- Problems with contact lenses or lens care products could result in serious injury to the eye. Patients should be cautioned that proper use and care of contact lenses and lens care products, including lens cases, are essential for the safe use of these products.
- The overall risk of ulcerative keratitis may be reduced by carefully following directions for lens care, including cleaning the lens case.

<sup>3</sup>New England Journal of Medicine, September 21, 1989; 321 (12), pp. 773-783

**Specific Instructions for Use and Warnings:**

- **Water Activity**

**Instructions for Use**

Do not expose contact lenses to water while wearing them.

**WARNING:**

Water can harbor microorganisms that can lead to severe infection, vision loss or blindness. If lenses have been submersed in water when participating in water sports or swimming in pools, hot tubs, lakes or oceans, the patient should be instructed to discard them and replace them with a new pair. The Eye Care Professional should be consulted for recommendations regarding wearing lenses during any activity involving water.

- **Soaking and Storing Your Lenses**

**Instructions for Use**

Use only fresh multi-purpose (contact lens disinfecting) solution each time the lenses are soaked (stored).

**WARNING:**

Do not reuse or “top off” old solution left in the lens case since solution reuse reduces effective lens disinfection and could lead to severe infection, vision loss, or blindness.



“Topping-Off” is the addition of fresh solution to solution that has been sitting the case.

- **Discard Date on Multi-Purpose Solution Bottle**

**Instructions for Use**

- Discard any remaining solution after the recommended time period indicated on the bottle of multi-purpose solution used for disinfecting and soaking the contact lenses.
- The Discard Date refers to the time that the patient can safely use contact lens care product after the bottle has been opened. It is not the same as the expiration date, which is the last date that the product is still effective before it is opened.

**WARNING:**

Using multi-purpose solution beyond the discard date could result in contamination of the solution and can lead to severe infection, vision loss, or blindness.

- To avoid contamination, DO NOT touch tip of container to any surface. Replace cap after using.
- To avoid contaminating the solution, DO NOT transfer to other bottles or containers.

- **Rub and Rinse Time**

**Instructions for Use**

To adequately disinfect the lenses, the patient should rub and rinse the lenses according to the recommended lens rubbing and rinsing times in the labeling of the multi-purpose solution.

**WARNING:**

- Rub and rinse lenses for the recommended amount of time to help prevent serious eye infections.
- Never use water, saline solution, or rewetting drops to disinfect the lenses. These solutions will not disinfect the lenses. Not using the recommended disinfectant can lead to severe infection, vision loss, or blindness.

- **Lens Case Care**

**Instructions for Use**

- Empty and clean contact lens cases with digital rubbing using fresh, sterile disinfecting solutions/contact lens cleaner. Never use water. Cleaning should be followed by rinsing with fresh, sterile disinfecting solutions (never use water) and wiping the lens cases with fresh, clean tissue is recommended. Never air dry or recap the lens case lids after use without any additional cleaning methods. If air drying, be sure that no residual solution remains in the case before allowing it to air dry.
- Replace the lens case according to the directions provided by the Eye Care Professional or the manufacturer’s labeling that accompanies the case.

– Contact lens cases can be a source of bacterial growth.

### **WARNING:**

Do not store lenses or rinse lens cases with water or any non-sterile solution. Only fresh multi-purpose solution should be used to prevent contamination of the lenses or lens case. Use of non-sterile solution can lead to severe infection, vision loss, or blindness.

## **PRECAUTIONS**

### **Special Precautions for Eye Care Professionals:**

- Due to the small number of patients enrolled in clinical investigation of lenses, all refractive powers, design configurations, or lens parameters available in the lens material are not evaluated in significant numbers. Consequently, when selecting an appropriate lens design and parameters, the Eye Care Professional should consider all characteristics of the lens that can affect lens performance and ocular health, including oxygen permeability, wettability, central and peripheral thickness, and optic zone diameter.

The potential impact of these factors on the patient's ocular health should be carefully weighed against the patient's need for refractive correction; therefore, the continuing ocular health of the patient and lens performance on the eye should be carefully monitored by the prescribing Eye Care Professional.

- Patients who wear these lenses to correct presbyopia using monovision may not achieve the best corrected visual acuity for either far or near vision. Visual requirements vary with the individual and should be considered when selecting the most appropriate type of lens for each patient.
- Fluorescein, a yellow dye, should not be used while the lenses are on the eyes. The lenses absorb this dye and become discolored. Whenever fluorescein is used in eyes, the eyes should be flushed with a sterile saline solution that is recommended for in-eye use.
- Eye Care Professionals should instruct the patient to remove lenses immediately if the eyes become red or irritated.

### **Eye Care Professionals should carefully instruct patients about the following care regimen and safety precautions:**

#### **Handling Precautions:**

- Before leaving the Eye Care Professional's office, the patient should be able to promptly remove the lenses or should have someone else available who can remove the lenses for him or her.
- DO NOT use if the sterile blister package is opened or damaged.
- Always wash and rinse hands before handling lenses. Do not get cosmetics, lotions, soaps, creams, deodorants, or sprays in the eyes or on the lenses. It

is best to put on lenses before putting on makeup. Water-based cosmetics are less likely to damage lenses than oil-based products.

- DO NOT touch contact lenses with the fingers or hands if the hands are not free of foreign materials, as microscopic scratches of the lenses may occur, causing distorted vision and/or injury to the eye.
- Carefully follow the handling, insertion, removal, and wearing instructions in the Patient Instruction Guide for these lenses and those prescribed by the Eye Care Professional.
- Always handle lenses carefully and avoid dropping them.
- Never use tweezers or other tools to remove lenses from the lens container unless specifically indicated for that use. Slide the lens up the side of the bowl until it is free of the container.
- Do not touch the lens with fingernails.
- Close supervision is necessary for the Therapeutic use of these lenses. Ocular medications used during treatment with a bandage lens should be closely monitored by the Eye Care Professional. In certain ocular conditions, only the Eye Care Professional will insert and remove the lenses. In these cases, patients should be instructed not to handle the lenses themselves.

### **Lens Wearing Precautions:**

- If the lens sticks (stops moving) on the eye, follow the recommended directions in “Care for Sticking (Non-Moving) Lenses”. The lens should move freely on the eye for the continued health of the eye. If non-movement of the lens continues, the patient should be instructed to immediately consult his or her Eye Care Professional.
- Never wear lenses beyond the period recommended by the Eye Care Professional.
- The patient should be advised to never allow anyone else to wear their lenses. They have been prescribed to fit their eyes and to correct their vision to the degree necessary. Sharing lenses greatly increases the chance of eye infections.
- If aerosol products, such as hair spray, are used while wearing lenses, exercise caution and keep eyes closed until the spray has settled.
- Avoid all harmful or irritating vapors and fumes while wearing lenses.

### **Lens Care Precautions:**

- Different solutions cannot always be used together and not all solutions are safe for use with all lenses. Use only recommended solutions.
- Never use solutions recommended for conventional hard contact lenses only.
- Chemical disinfection solutions should not be used with heat unless

specifically indicated on product labeling for use in both heat and chemical disinfection.

- Always use fresh, unexpired lens care solutions and lenses.
- Do not change solution without consulting with your Eye Care Professional.
- Always follow directions in the package inserts for the use of contact lens solutions.
- Use only a chemical (not heat) lens care system. Use of a heat (thermal) care system can damage these lenses.
- Sterile unpreserved solutions, when used, should be discarded after the time specified in the directions.
- Do not use saliva or anything other than the recommended solutions for lubricating or wetting lenses.
- Always keep the lenses completely immersed in the recommended storage solution when the lenses are not being worn (stored). Prolonged periods of drying will reduce the ability of the lens surface to return to a wettable state. Follow the lens care directions in "Care For A Dried Out (Dehydrated) Lens" if lens surface does become dried out.

### **Other Topics to Discuss with Patients:**

- Always contact the Eye Care Professional before using any medicine in the eyes.
- Certain medications, such as antihistamines, decongestants, diuretics, muscle relaxants, tranquilizers, and those for motion sickness may cause dryness of the eye, increased lens awareness, or blurred vision. Should such conditions exist, proper remedial measures should be prescribed. Depending on the severity, this could include the use of lubricating drops that are indicated for use with soft contact lenses or the temporary discontinuance of contact lens wear while such medication is being used.
- Oral contraceptive users could develop visual changes or changes in lens tolerance when using contact lenses. Patients should be cautioned accordingly.
- As with any contact lens, follow-up visits are necessary to assure the continuing health of the patient's eyes. The patient should be instructed as to a recommended follow-up schedule.

### **Who Should Know That the Patient is Wearing Contact Lenses?**

- Patients should inform all doctors (Health Care Professionals) about being a contact lens wearer.
- Patients should always inform their employer of being a contact lens wearer. Some jobs may require use of eye protection equipment or may require that the patient not wear contact lenses.

# ADVERSE REACTIONS

**The patient should be informed that the following problems may occur when wearing contact lenses:**

- The eye may burn, sting and/or itch.
- There may be less comfort than when the lens was first placed on the eye.
- There may be a feeling of something in the eye (foreign body, scratched area).
- There may be the potential for some temporary impairment due to peripheral infiltrates, peripheral corneal ulcers, and corneal erosion. There may be the potential for other physiological observations, such as local or generalized edema, corneal neovascularization, corneal staining, injection, tarsal abnormalities, iritis and conjunctivitis, some of which are clinically acceptable in low amounts.
- There may be excessive watering, unusual eye secretions or redness of the eye.
- Poor visual acuity, blurred vision, rainbows or halos around objects, photophobia, or dry eyes may also occur if the lenses are worn continuously or for too long a time.
- The patient should be instructed to conduct a simple 3-part self-examination at least once a day. They should ask themselves:
  - How do the lenses feel on my eyes?
  - How do my eyes look?
  - Have I noticed a change in my vision?

If the patient reports any problems, he or she should be instructed to **IMMEDIATELY REMOVE THE LENS**. If the problem or discomfort stops, the patient should discard the lens and place a new fresh lens on the eye.

If after inserting the new lens, the problem continues, the patient should be directed to **IMMEDIATELY REMOVE THE LENS AND CONTACT HIS OR HER EYE CARE PROFESSIONAL**.

The patient should be instructed **NOT** to use a new lens as self-treatment for the problem.

The patient should be advised that when any of the above symptoms occur, a serious condition such as infection, corneal ulcer, neovascularization or iritis may be present. He or she should be instructed to seek immediate professional identification of the problem and prompt treatment to avoid serious eye damage.

# GENERAL FITTING GUIDELINES

## A. Patient Selection:

Patients selected to wear these lenses should be chosen based on:

- Motivation to wear lenses
- Ability to follow instructions regarding lens wear care
- General health
- Ability to adequately handle and care for the lenses
- Ability to understand the risk and benefits of lens wear

Patients who do not meet the above criteria should not be provided with contact lenses.

## B. Pre-fitting Examination:

Initial evaluation of the patient should begin with a thorough case history to determine if there are any contraindications to contact lens wear. During the case history, the patient's visual needs and expectations should be determined as well as an assessment of their overall ocular, physical, and mental health.

Preceding the initial selection of trial contact lenses, a comprehensive ocular evaluation should be performed that includes, but is not limited to, the measurement of distance and near visual acuity, distance and near refractive prescription (including determining the preferred reading distance for presbyopes), keratometry and biomicroscopic evaluation.

Based on this evaluation, if it is determined that the patient is eligible to wear these lenses, the Eye Care Professional should proceed to the appropriate lens fitting instruction outlined below.

## C. Initial Power Determination

A spectacle refraction should be performed to establish the patient's baseline refractive status and to guide in the selection of the appropriate lens power. Remember to compensate for vertex distance if the refraction is greater than  $\pm 4.00D$ .

## D. Base Curve Selection (Trial Lens Fitting)

The following trial lenses should be selected for patients regardless of keratometry readings. However, corneal curvature measurements should be performed to establish the patient's baseline ocular status.

- **ACUVUE OASYS®:** 8.4 mm/14.0 mm
- **ACUVUE OASYS® for ASTIGMATISM:** 8.6 mm/14.5 mm
- **ACUVUE OASYS® for PRESBYOPIA:** 8.4 mm/14.3 mm

The trial lenses should be placed on each of the patient's eyes and evaluated after the patient has adjusted to the lenses.

### 1. Criteria of a Properly Fit Lens

A properly fit lens will center and completely cover the cornea (i.e., no limbal exposure), have sufficient movement to provide tear exchange under the contact lens with the blink, and be comfortable. The lens should move freely when manipulated digitally with the lower lid, and then return to its properly centered position when released.

### 2. Criteria of a Flat Fitting Lens

A flat fitting lens may exhibit one or more of the following characteristics: decentration, incomplete corneal coverage (i.e., limbal exposure), excessive movement with the blink and/or edge standoff. If the lens is judged to be flat fitting, it should not be dispensed to the patient.

### 3. Criteria of a Steep Fitting Lens

A steep fitting lens may exhibit one or more of the following characteristics: insufficient movement with the blink, conjunctival indentation, and resistance when pushing the lens up digitally with the lower lid. If the lens is judged to be steep fitting, it should not be dispensed to the patient.

If the initial trial base curve is judged to be flat or steep fitting, the alternate base curve, if available, should be trial fit and evaluated after the patient has adjusted to the lens. The lens should move freely when manipulated digitally with lower lid, and then return to a properly centered position when released. If resistance is encountered when pushing the lens up, the lens is fitting tightly and should not be dispensed to the patient.

## **E. Final Lens Power (Spherical)**

A spherical over-refraction should be performed to determine the final lens power after the lens fit is judged acceptable. The spherical over-refraction should be combined with the trial lens power to determine the final lens prescription. The patient should experience good visual acuity with the correct lens power unless there is excessive residual astigmatism.

Example 1	
Diagnostic lens:	-2.00D
Spherical over-refraction:	-0.25D
Final lens power:	-2.25D

Example 2	
Diagnostic lens:	-2.00D
Spherical over-refraction:	+0.25D
Final lens power:	-1.75D

If vision is acceptable, perform a slit lamp examination to assess adequate fit (centration and movement). If fit is acceptable, dispense the lenses instructing the patient to return in one week for reassessment (see dispensing and follow-up information in PATIENT MANAGEMENT).

**All patients should be supplied with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at [www.acuvue.com](http://www.acuvue.com).**

## TORIC FITTING GUIDELINES

Although most aspects of the fitting procedure are identical for all types of soft contact lenses, including torics, there are some additional steps and/or rules to follow to assure the proper fit of toric lenses.

The only new steps you must follow in prescribing ACUVUE OASYS® for ASTIGMATISM contact lenses are that you must determine the stability, repeatability and drift angle of the lens axis so that you can prescribe the correct lens axis for your patient.

### A. How to Determine Lens Cylinder and Axis Orientation

#### 1. Locate the Orientation Marks

To help determine the proper orientation of the toric lens, you'll find two primary marks about 1 mm from the lens edge representing the vertical position on opposite ends of the lens at 6 and 12 o'clock (Fig. 1). Because of the lens' ballasting system, either mark can represent the vertical position – there is no “top” and “bottom” as in a prism-ballasted lens. You don't need to view both marks to assess orientation; simply look for the 6 o'clock mark as you would with a prism-ballasted lens.



**Figure 1**

You'll need a biomicroscope and a 1 mm or 2 mm parallelepiped beam to highlight the marks when the lens is fitted to the eye. There are a number of techniques you can use to improve the visibility of the 6 o'clock mark. Using a parallelepiped beam and medium magnification (10x or 15x), slowly pan down the lens, looking just below the direct illumination at the retroilluminated area. Backlighting the mark this way should make it more visible. Sometimes manipulating the lower lid may be necessary to uncover the mark.

#### 2. Observe Lens Rotation and Stability

Observe the position and stability of the “bottom” mark. It usually stabilizes at the 6 o'clock position. If it does, calculation of the lens power will be straightforward. The 6 o'clock position is not a “must”; however, the absolute requirement is that the axis position be stable and repeatable.



The mark may stabilize somewhat left or right (drift) of the vertical meridian and still enable you to fit a toric lens for that eye, as long as the lens always returns to the same “drift axis” position after settling. The deviation can be compensated for in the final prescription. Your objective is to ensure that whatever position the initial lens assumes near 6 o’clock, this position must be stable and repeatable. With full eye movement or heavy blink, you may see the marks swing away, but they must return quickly to the original stable position. If the lens does not return quickly, you may need to select a different lens.

### **Assessing Rotation**

Imagine the eye as a clock dial and every hour represents a 30° interval. If the orientation mark of the initial lens stabilizes somewhat left or right of the vertical position, the final lens will orient on the eye with the same deviation. You can use an axis reticule in the slit lamp or use a line-scribed lens in a spectacle trial frame to measure or estimate the “drift angle” of the cylinder axis.

To compensate for this “drift”, measure or estimate the “drift”, then add or subtract it from the refractive axis to determine the correct cylinder axis. Use the LARS (Left Add, Right Subtract) method to determine which direction to compensate.

## **B. How to Determine the Final Lens Power**

When the diagnostic lens has its axis aligned in the same meridian as the patient’s refractive axis, a spherocylindrical over-refraction may be performed and visual acuity determined. However, in the case of crossed axes, such as when the diagnostic lens axis is different from the patient’s refractive axis, it is not advisable to over-refract because of the difficulty in computing the resultant power. In fitting contact lenses, it is customary to prescribe the full power in the sphere. In the cylinder, however, any lens rotation is visually disturbing to the patient, so it’s more practical to prescribe as weak a cylinder as possible. So, here is how to determine the final lens power.

### **For the Sphere:**

If sphere alone or combined sphere and cylinder Rx  $> \pm 4.00D$ , compensate for vertex distance. If sphere alone or combined sphere and cylinder Rx  $\leq \pm 4.00D$ , vertex compensation is not necessary.

### **For the Cylinder:**

Adjust the axis by the drift angle using LARS. Choose a cylinder that is  $\leq 0.25D$  from the refractive cylinder.

### **Case Examples:**

#### **Example 1**

Manifest (spectacle) refraction:

O.D.  $-2.50 -1.25 \times 180$  20/20

O.S.  $-2.00 -1.00 \times 180$  20/20

Choose a diagnostic lens for each eye with an axis as close to 180° as possible. Place the lens on each eye and allow a minimum of 3 minutes for

it to equilibrate, based on the patient's initial response to the lens. If the lens has not yet stabilized, recheck until stable.

Check the orientation of the axis mark. If the bottom axis mark is in the 6 o'clock position on both eyes, choose the appropriate cylinder as listed previously. If the lens has not yet stabilized, recheck until stable.

Here is the Rx Prescribed:

O.D. -2.50 -1.25 x 180

O.S. -2.00 -0.75 x 180

## **Example 2**

Manifest (spectacle) refraction:

O.D. -3.00 -1.00 x 90 20/20

O.S. -4.75 -2.00 x 90 20/20

Choose diagnostic lenses of -3.00 -0.75 x 90 for the right eye and -4.50 -1.75 x 90 for the left eye, the nearest lenses available to the spherical power and axis needed. Place the lens on each eye and allow a minimum of 3 minutes for it to equilibrate, based on the patient's initial response to the lens. If the lens has not yet stabilized, recheck until stable. The orientation mark on the right lens rotates left from the 6 o'clock position by 10°.

The fitting indicates the following:

### **Right Eye:**

Compensate the 10° axis drift by adding it to the manifest refraction axis.

Here is the Rx prescribed:

O.D. -3.00 -0.75 x 100

### **Left Eye**

The lens on the left eye shows good centration, movement and a consistent tendency for the mark to drift right by 10° from the 6 o'clock position following a forced blink. Since the manifest refraction called for a power of -4.75D, adjust for the vertex distance and reduce the sphere by 0.25D and prescribe the -1.75D cylinder. Compensate for the 10° axis drift by subtracting it from the manifest refraction.

Here is the Rx Prescribed:

O.S. -4.50 -1.75 x 80

If vision is acceptable, perform a slit lamp examination to assess adequate fit (centration and movement). If fit is acceptable, dispense the lenses instructing the patient to return in one week for reassessment (see dispensing and follow up information in PATIENT MANAGEMENT).

**All patients should be supplied with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at [www.acuvue.com](http://www.acuvue.com).**

# MULTIFOCAL FITTING GUIDELINES

## A. Presbyopic Needs Assessment & Patient Education

Multifocal contact lenses may produce compromise to vision under certain circumstances and the patient should understand that they might not find their vision acceptable in specific situations (i.e., reading a menu in a dim restaurant, driving at night in rainy/foggy conditions, etc.). Therefore, caution should be exercised when the patient is wearing the correction for the first time until they are familiar with the vision provided in visually challenging environments. Occupational and environmental visual demands should be considered. If the patient requires critical visual acuity and stereopsis, it should be determined by trial whether this patient can function adequately with the ACUVUE OASYS® for PRESBYOPIA contact lenses. Wear may not be optimal for activities such as:

1. visually demanding situations such as operating potentially dangerous machinery or performing other potentially hazardous activities; and
2. driving automobiles (e.g., driving at night). Patients who cannot pass their state driver's license requirements with these lenses should be advised to not drive with this correction, OR may require that additional over-correction be prescribed.

These lenses are not recommended for patients who have  $-1.00D$  or greater of refractive cylinder as this level of uncorrected cylinder may lead to additional visual compromise.

These lenses are available in the following ADD powers:

- Lens "LOW" = "low" near ADD lens (Max +1.25 ADD)
- Lens "MID" = "medium" near ADD lens (Max +1.75 ADD)
- Lens "HGH" = "high" near ADD lens (Max +2.50 ADD)

## B. Fitting Instructions

### 1. Determine the following:

- Eye dominance (the methods described in MONOVISION FITTING GUIDELINES may be used)
- Spherical equivalent distance prescription (vertex corrected if necessary and rounded to less minus if between powers)
- Near ADD

### 2. Select the initial trial lens as follows:

- For each eye select the trial lens distance power that is closest to the patient's distance spherical equivalent.

- Select the near power of the lens based on the patient's ADD range as follows:

ADD: +0.75 to +1.25 use a “LOW” near ADD lens on each eye

ADD: +1.50 to +1.75 use a “MID” near ADD lens on each eye

ADD: +2.00 to +2.50 use a “HGH” near ADD lens on each eye

### **3. Allow the lens to settle for a minimum 10 minutes.**

### **4. Assess distance and near vision binocularly and monocularly.**

- Demonstrate the vision under various lighting conditions (normal and decreased illumination) and at distance, intermediate and near.
- Make adjustments in power as necessary (see Multifocal Troubleshooting below). The use of hand-held trial lenses is recommended.
- If distance and near vision are acceptable, perform a slit lamp examination to assess adequate fit (centration and movement). If fit is acceptable, dispense the lenses instructing the patient to return in one week for reassessment (see dispensing and follow-up information in PATIENT MANAGEMENT).

## **C. Multifocal Troubleshooting**

### **Unacceptable Near Vision:**

Determine the amount of additional plus, or less minus, over one or both eyes that is acceptable, while checking the effect on distance and near vision. If vision is still not acceptable, change the non-dominant eye to the next highest ADD power.

### **Unacceptable Distance Vision:**

Determine the amount of additional minus, or less plus, over one or both eyes that is acceptable while checking the effect on distance and near vision. If vision is still not acceptable, change the dominant eye to the next lowest ADD power. If the patient is wearing two low ADD lenses, change the dominant eye to a sphere lens with a power equal to the spherical equivalent distance prescription.

### **Unacceptable Distance and Near Vision:**

Determine the amount of additional plus and/or minus over one or both eyes that is acceptable while checking the effect on distance and near vision. If additional plus and/or minus is not required, change the lens power in the dominant eye to the next lowest ADD power and the lens power in the non-dominant eye to the next highest ADD power, if applicable.

**All patients should be supplied with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at [www.acuvue.com](http://www.acuvue.com).**

# MONOVISION FITTING GUIDELINES

## A. Patient Selection

### Monovision Needs Assessment

For a good prognosis, the patient should have adequately corrected distance and near visual acuity in each eye. The amblyopic patient or the patient with significant astigmatism (greater than 1.00D) in one eye may not be a good candidate for monovision correction with these lenses.

Occupational and environmental visual demands should be considered. If the patient requires critical vision (visual acuity and stereopsis), it should be determined by trial whether this patient can function adequately with monovision correction. Monovision contact lens wear may not be optimal for activities such as:

1. visually demanding situations such as operating potentially dangerous machinery or performing other potentially hazardous activities; and
2. driving automobiles (e.g., driving at night). Patients who cannot pass their state driver's license requirements with monovision correction should be advised to not drive with this correction, OR may require that additional over-correction be prescribed.

### Patient Education

All patients do not function equally well with monovision correction. Patients may not perform as well for certain tasks with this correction as they have with spectacles (multifocal, bifocal, trifocal, readers, progressives). Each patient should understand that monovision, as well as other presbyopic alternatives, can create a vision compromise that may reduce visual acuity and depth perception for distance and near tasks. Therefore, caution should be exercised when the patient is wearing the correction for the first time until they are familiar with the vision provided in visually challenging environments (e.g., reading a menu in a dim restaurant, driving at night in rainy/foggy conditions, etc.). During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

## B. Eye Selection

Generally, the non-dominant eye is corrected for near vision. The following two methods for eye dominance can be used.

### 1. Ocular Preference Determination Methods

Method 1: Determine which eye is the "sighting eye." Have the patient point to an object at the far end of the room. Cover one eye. If the patient is still pointing directly at the object, the eye being used is the dominant (sighting) eye.

Method 2: Determine which eye will accept the added power with the least reduction in vision. Place a hand-held trial lens equal to the spectacle near ADD in front of one eye and then the other while the distance refractive error correction is in place for both eyes. Determine whether the patient functions best with the near ADD lens over the right or left eye.

Other methods include the refractive error method and the visual demands method.

## **2. Refractive Error Method**

For anisometropic correction, it is generally best to fit the more hyperopic (less myopic) eye for distance and the more myopic (less hyperopic) eye for near.

## **3. Visual Demands Method**

Consider the patient's occupation during the eye selection process to determine the critical vision requirements. If a patient's gaze for near tasks is usually in one direction, correct the eye on that side for near.

Example: A secretary who places copy to the left side of the desk will function best with the near lens on the left eye.

# **C. Special Fitting Characteristics**

## **1. Unilateral Lens Correction**

There are circumstances where only one contact lens is required. As an example, an emmetropic patient would only require a near lens while a bilateral myope may only require a distance lens.

Example: A presbyopic emmetropic patient who requires a +1.75D ADD would have a +1.75D lens on the near eye and the other eye left without a lens. A presbyopic patient requiring a +1.50D ADD who is -2.50D myopic in the right eye and -1.50D myopic in the left eye may have the right eye corrected for distance and the left uncorrected for near.

## **2. Near ADD Determination**

Always prescribe the lens power for the near eye that provides optimal near acuity at the midpoint of the patient's habitual reading distance. However, when more than one power provides optimal reading performance, prescribe the least plus (most minus) of the powers.

## **3. Trial Lens Fitting**

A trial fitting is performed in the office to allow the patient to experience monovision correction. Lenses are fit according to the GENERAL FITTING GUIDELINES for base curve selection in this Package Insert.

Case history and standard clinical evaluation procedure should be used to determine the prognosis. Determine the distance correction and the near correction. Next determine the near ADD. With trial lenses of the proper power in place, observe the reaction to this mode of correction.

Allow the lenses to settle for about 20 minutes with the correct power lenses in place. Walk across the room and have the patient look at you. Assess the patient's reaction to distance vision under these circumstances. Then have the patient look at familiar near objects such as a watch face or fingernails. Again assess the reaction. As the patient continues to look around the room at both near and distance objects, observe the reactions. Only after these vision tests are completed should the patient be asked to read print. Evaluate the patient's reaction to large print (e.g., typewritten copy) at first and then graduate to newsprint and finally smaller type sizes.

After the patient's performance under the above conditions is completed, tests of visual acuity and reading ability under conditions of moderately dim illumination should be attempted.

An initial unfavorable response in the office, while indicative of a guarded prognosis, should not immediately rule out a more extensive trial under the usual conditions in which a patient functions.

#### **4. Adaptation**

Visually demanding situations should be avoided during the initial wearing period. A patient may at first experience some mild blurred vision, dizziness, headaches, and a feeling of slight imbalance. You should explain the adaptational symptoms to the patient. These symptoms may last for a brief minute or for several weeks. The longer these symptoms persist, the poorer the prognosis for successful adaptation.

To help in the adaptation process, the patient can be advised to first use the lenses in a comfortable familiar environment such as in the home.

Some patients feel that automobile driving performance may not be optimal during the adaptation process. This is particularly true when driving at night. Before driving a motor vehicle, it may be recommended that the patient be a passenger first to make sure that their vision is satisfactory for operating an automobile. During the first several weeks of wear (when adaptation is occurring), it may be advisable for the patient to only drive during optimal driving conditions. After adaptation and success with these activities, the patient should be able to drive under other conditions with caution.

#### **D. Other Suggestions**

The success of the monovision technique may be further improved by having the patient follow the suggestions below:

- Have a third contact lens (distance power) to use when critical distance viewing is needed.
- Have a third contact lens (near power) to use when critical near viewing is needed.
- Having supplemental spectacles to wear over the monovision contact lenses

for specific visual tasks may improve the success of monovision correction. This is particularly applicable for those patients who cannot pass state drivers licensing requirements with monovision correction.

- Make use of proper illumination when carrying out visual tasks.

Monovision fitting success can be improved by the following suggestions:

- Reverse the distance and near eyes if a patient is having trouble adapting.
- Refine the lens powers if there is trouble with adaptation. Accurate lens power is critical for presbyopic patients.
- Emphasize the benefits of clear near vision and straight ahead and upward gaze with monovision.

The decision to fit a patient with a monovision correction is most appropriately left to the Eye Care Professional in conjunction with the patient after carefully considering the patient's needs.

**All patients should be supplied with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at [www.acuvue.com](http://www.acuvue.com).**

## PATIENT MANAGEMENT

### Dispensing Visit

- PROVIDE THE PATIENT WITH A COPY OF THE PATIENT INSTRUCTION GUIDE FOR THESE LENSES. REVIEW THESE INSTRUCTIONS WITH THE PATIENT SO THAT HE OR SHE CLEARLY UNDERSTANDS THE PRESCRIBED WEARING AND REPLACEMENT SCHEDULE (DISPOSABLE OR FREQUENT REPLACEMENT).
- Recommend an appropriate cleaning and disinfecting system and provide the patient with instructions regarding proper lens care. Chemical or hydrogen peroxide disinfection is recommended.
- Schedule a follow-up examination.

### Follow-up Examinations

- Follow-up care (necessary to ensure continued successful contact lens wear) should include routine periodic progress examinations, management of specific problems, if any, and a review with the patient of the wear schedule, lens replacement schedule, and proper lens care and handling procedures.
- Recommended Follow-up Examination Schedule (complications and specific problems should be managed on an individual patient basis):
  1. One week from the initial lens dispensing to patient
  2. One month post-dispensing
  3. Every three to six months thereafter



NOTE: More frequent or additional follow-up visits may be recommended for patients on an extended wear schedule.

- Preferably, at the follow-up visits, lenses should be worn for at least six hours. If the lenses are being worn for continuous wear, the examination should be performed as early as possible on the morning following overnight wear.
- Recommended Procedures for Follow-Up Visits:
  1. Solicit and record patient's symptoms, if any.
  2. Measure visual acuity monocularly and binocularly at distance and near with the contact lenses.
  3. Perform an over-refraction at distance and near to check for residual refractive error.
  4. With the biomicroscope, judge the lens fitting characteristics (as described in the GENERAL FITTING GUIDELINES) and evaluate the lens surface for deposits and damage.
  5. Following lens removal, examine the cornea and conjunctiva with the biomicroscope and fluorescein (unless contraindicated).
    - The presence of vertical corneal striae in the posterior central cornea and/or corneal neovascularization is indicative of excessive corneal edema.
    - The presence of corneal staining and/or limbal-conjunctival hyperemia can be indicative of an unclean lens, a reaction to solution preservatives, excessive lens wear, and/or a poorly fitting lens.
    - Papillary conjunctival changes may be indicative of an unclean and/or damaged lens.
  6. Periodically perform keratometry and spectacle refractions. The values should be recorded and compared to the baseline measurements.

**If any observations are abnormal, use professional judgment to alleviate the problem and restore the eye to optimal conditions. If the criteria for successful fit are not satisfied during any follow-up examinations, repeat the patient's trial fitting procedure and refit the patient.**

## WEARING SCHEDULE

The wearing and replacement schedules should be determined by the Eye Care Professional. Regular checkups, as determined by the Eye Care Professional, are also extremely important.

### **For Daily Wear:**

Patients tend to overwear the lenses initially. The Eye Care Professional should emphasize the importance of adhering to the initial maximum wearing schedule. Maximum wearing time should be determined by the Eye Care Professional based upon the patient's physiological eye condition, because individual response to contact lenses varies.

The maximum suggested wearing time for these lenses is:

<b>DAY</b>	<b>HOURS</b>
1	6-8
2	8-10
3	10-12
4	12-14
5 and after	all waking hours

### **For Extended Wear:**

It is recommended that the contact lens wearer first be evaluated on a daily wear schedule. If successful, then a gradual introduction of extended wear can be followed as determined by the prescribing Eye Care Professional.

These lenses have been approved for extended wear up to 6 nights/7 days of continuous wear. Not all patients can achieve the maximum wear time.

**For Therapeutic** lens wear, close supervision by the Eye Care Professional is necessary. These lenses can be worn for extended wear for up to 6 nights/7 days of continuous wear. The Eye Care Professional should determine the appropriate wearing time and provide specific instructions to the patient regarding lens care, insertion, and removal.

## **REPLACEMENT SCHEDULE**

### **For Lenses Prescribed for Frequent Replacement:**

When prescribed for daily wear (frequent replacement), it is recommended that the lenses be discarded and replaced with a new lens every 2 weeks. However, the Eye Care Professional is encouraged to determine an appropriate replacement schedule based upon the response of the patient.

### **For Lenses Prescribed for Disposable Wear:**

When prescribed for disposable wear, the replacement schedule should be determined by the Eye Care Professional based upon the patient's history and their ocular examination, as well as the practitioner's experience and clinical judgment.

Once removed, it is recommended that the lens remain out of the eye for a period of rest of overnight or longer and be discarded in accordance with the prescribed wearing schedule. The Eye Care Professional should examine the patient during the early stages of extended wear.

# LENS CARE DIRECTIONS

When lenses are dispensed, the Eye Care Professional should provide the patient with appropriate and adequate warnings and instructions in accordance with the individual patient's lens type and wearing schedule. The Eye Care Professional should recommend an appropriate care system tailored to the patient's individual requirements.

For complete information concerning contact lens handling, care, cleaning, disinfecting and storage, refer to the Patient Instruction Guide for these lenses. Copies are available for download at [www.acuvue.com](http://www.acuvue.com).

## **For Lenses Prescribed for Frequent Replacement Wear:**

The Eye Care Professional should review with the patient, lens care directions for cleaning, disinfecting and storing, including both basic lens care information and specific instructions on the lens care regimen recommended for the patient.

## **For Lenses Prescribed for Disposable Wear:**

The Eye Care Professional should review with patients that no cleaning or disinfection is needed with disposable lenses. Patients should always dispose of lenses when they are removed and have replacement lenses or spectacles available. Lenses should only be cleaned, rinsed, and disinfected on an emergency basis when replacement lenses or spectacles are not available.

## **Care for a Dried Out (Dehydrated) Lens**

If the frequent replacement lens is off the eye and exposed to air from 30 minutes to 1 hour or more, its surface will become dry and gradually become non-wetting. If this should occur, discard the lens and use a new one.

## **Care for Sticking (Non-Moving) Lenses**

If the lens sticks (stops moving), the patient should be instructed to apply a few drops of the recommended lubricating or rewetting solution directly to the eye and wait until the lens begins to move freely on the eye before removing it. If non-movement of the lens continues after a few minutes, the patient should **immediately** contact the Eye Care Professional.

# EMERGENCIES

The patient should be informed that if chemicals of any kind (household products, gardening solutions, laboratory chemicals, etc.) are splashed into the eyes, the patient should: **FLUSH EYES IMMEDIATELY WITH TAP WATER AND IMMEDIATELY CONTACT THE EYE CARE PROFESSIONAL OR VISIT A HOSPITAL EMERGENCY ROOM WITHOUT DELAY.**

## HOW SUPPLIED

Each sterile lens is supplied in a foil-sealed plastic package containing buffered saline solution with methyl ether cellulose. The plastic package is marked with the following:

- **ACUVUE OASYS®**: base curve, power, diameter, lot number, and expiration date
- **ACUVUE OASYS® for ASTIGMATISM**: base curve, power, diameter, cylinder, axis, lot number, and expiration date
- **ACUVUE OASYS® for PRESBYOPIA**: base curve, power, diameter, ADD, lot number, and expiration date

## REPORTING OF ADVERSE REACTIONS

All serious adverse experiences and adverse reactions observed in patients wearing these lenses or experienced with the lenses should be reported to:

Johnson & Johnson Vision Care, Inc.  
7500 Centurion Parkway  
Jacksonville, FL 32256  
USA  
Tel: 1-800-843-2020  
[www.acuvue.com](http://www.acuvue.com)



©Johnson & Johnson Vision Care Companies 2015  
In Canada: Johnson & Johnson Vision Care, division of Johnson & Johnson, Inc.  
In USA: Johnson & Johnson Vision Care, Inc.  
Printed in USA  
Revision date: 06/15  
Revision number: AO-06-15-01

ACUVUE OASYS® and HYDRACLEAR® are trademarks of  
Johnson & Johnson Vision Care Companies.